


REMOTE KEY FOB TRANSMITTER LOCATIONS



SJ1718

1. Keyless vehicle module.
2. Cabin front transmitter.
3. Exterior door handle transmitters.
4. Cabin rear transmitter.
5. Luggage compartment interior transmitter.
6. Luggage compartment exterior transmitter.

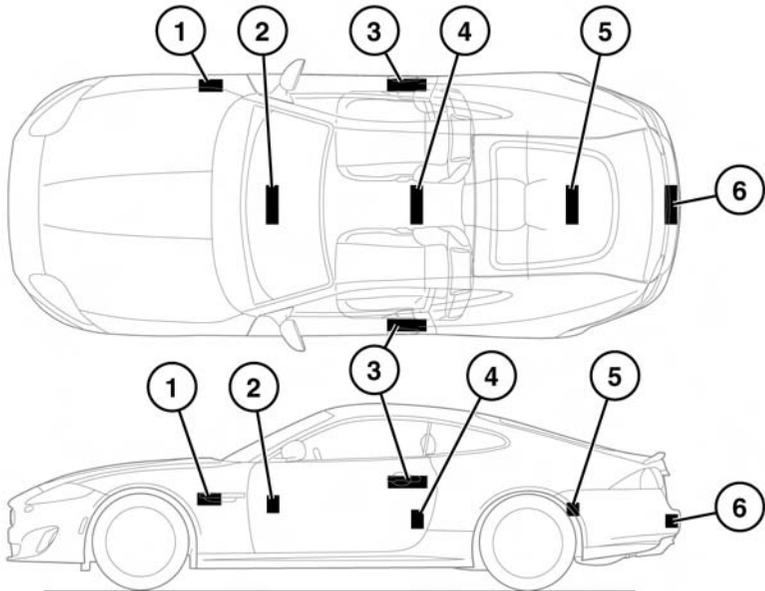

Any person fitted with an implanted medical device should ensure that the device is kept at a distance of at least 22 cm (8.7 inches) away from any transmitter mounted in the vehicle. This is to avoid any possibility of interference between the system and device.